

CERTIFICATE OF ANALYSIS

Product Name	(Ala1)-PAR-4 (1-6) amide, Cat.#: 311352
Lot No.	MTFB21232-261014
Sequence	AYPGKF-NH2
Dissolution condition	100%H2O
Modification	N/A
Molecular Weight (MW)	680.79
Storage	-20°C

Test Items	Specifications	Results
MW by MS	680.60	Conforms
Purity by HPLC	>95%	99.651%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20.0mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Oct/28/2026


Quality Assurance Department



Sample Information

Order ID	:MTFB21232		
Name	:(Ala1)-PAR-4 (1-6) amide, Cat.#: 311352		
Sequence	:AYPGKF-NH2		
Lot. No	:MTFB21232-261014		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 15ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	10
30.00	Pumps	B.Conc	40
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	10
50.00	Controller	Stop	

Chromatogram

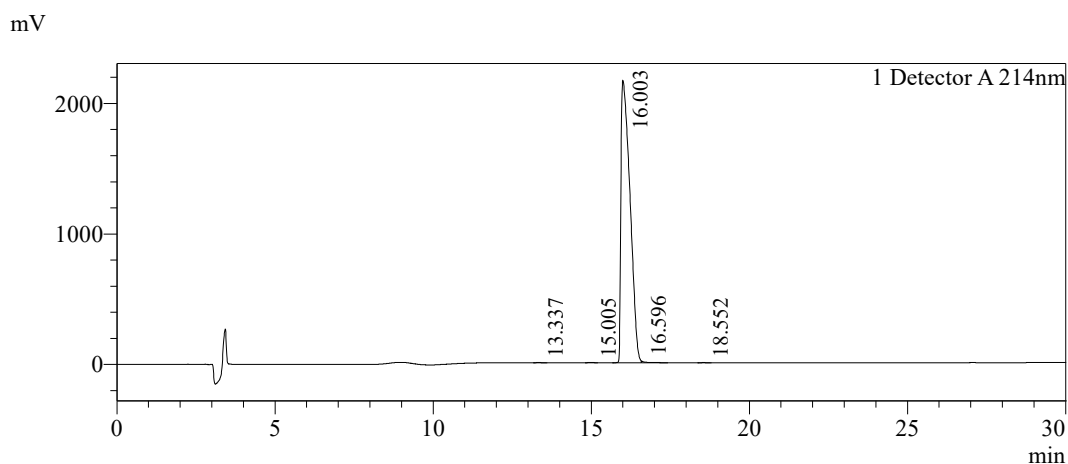


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	13.337	15735	2080	0.036
2	15.005	18338	2317	0.042
3	16.003	43148774	2161882	99.651
4	16.596	108292	12625	0.250
5	18.552	8729	961	0.020
Total		43299868	2179865	100.000

MS Spectrum

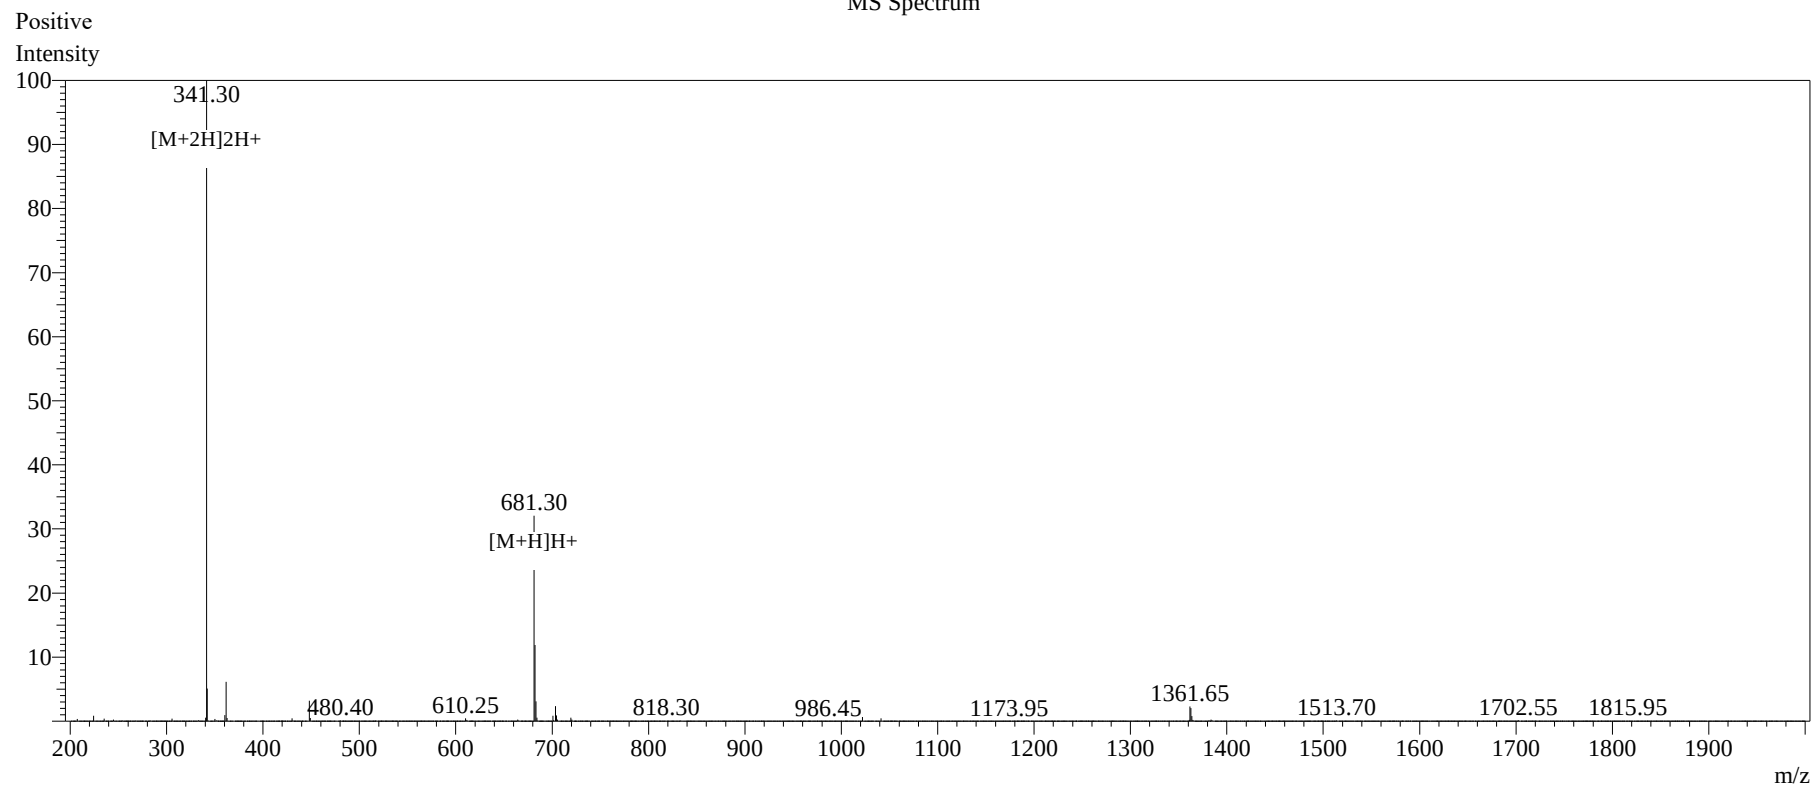

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/10/27 16:18:32	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH
Order ID	:MTFB21232				
Name	:(Ala1)-PAR-4 (1-6) amide, Cat.#: 311352				
Sequence	:AYPGKF-NH2				
Lot.No	:MTFB21232-261014				
Theoretical	:680.79				
Observed	:680.60				