

CERTIFICATE OF ANALYSIS

Product Name Antigenic peptides of SSA, Cat.#: 318956

Lot No. GTA34751-1-1123

Sequence AVALREYRKKMDIPA

Dissolution condition 100%H2O

Length 15AA

Modification N/A

Molecular Weight (MW) 1761.08

Storage -20°C

Test Items	Specifications	Results
MW by MS	1761.10	Conforms
Purity by HPLC	>70%	97.315%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	5mg	5.0mg

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:

Quality Assurance Department

Nov./30/2022



Sample Information

Order ID :GTA34751-1

Name :N/A

Sequence :AVALREYRKKMDIPA Lot. No :GTA34751-1-1123

Pump A :0.1% Trifluoroacetic in 100% water Pump B :0.1% Trifluoroacetic in 100% acetonitrile

Total Flow :1ml/min Wavelength :214nm


Analytial column type :YMC-Triart C18(4.6*250mm*5um)

Dissolution method :100%H2O Inj. Volume :25ul

Time Module Action Value 0.01 Pumps B.Conc 15 B.Conc 25.00 **Pumps** 40 33.00 Pumps B.Conc 100 38.00 Pumps B.Conc 100 40.00 Pumps B.Conc 15 50.00 Controller Stop

Chromatogram



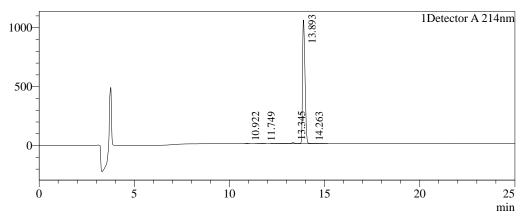


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%				
1	10.922	19516	2755	0.200				
2	11.749	18814	1808	0.193				
3	13.345	165496	9327	1.696				
4	13.893	9494556	1049151	97.315				
5	14.263	58156	1993	0.596				
Total		9756537	1065035	100.000				



MS Spectrum

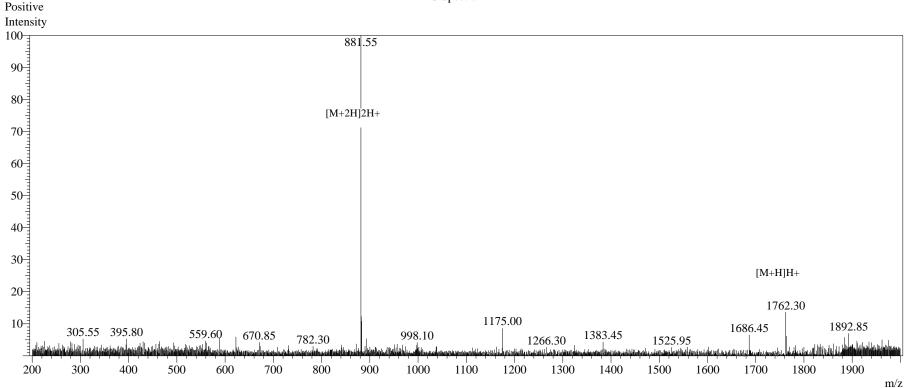

Sample Information

Dissolution method Date Acquired	:15% ACN+85% H2O :2022/11/25 09:47:39	Interface Nebulizing Gas Flow	:ESI :1.50L/min	Prerod Bias Detector	:+4.5kv :-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

:GTA34751-1 Order ID

:N/A Name

Sequence Lot.No :AVALREYRKKMDIPA

:GTA34751-1-1123 Theoretical :1761.08

Observed :1761.10