

CERTIFICATE OF ANALYSIS

Product Name	Cagrilintide, Cat.#: 319572 (TFA removed)
Lot No.	MTFA32213-1212
Sequence	{Eicosanedioic acid- γ -Glu}- KC*NTATC*ATQRLAEFLRHSSNNFGPILPPTNVGSNTP-NH2 (Acetate Salt)
Dissolution condition	100%H2O
Length	38AA
Modification	Disulfide bridge: Cys3-Cys8; acetate salt
Molecular Weight (MW)	4409.01
Storage	-20°C

Test Items	Specifications	Results
MW by MS	4409.80	Conforms
Purity by HPLC	>98%	99.396%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	1g	5.0mg*200

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Dec/17/2024




Sample Information

Order ID :MTFA32213
 Name :Cagrilintide
 Sequence :{Eicosanedioic acid- γ -Glu}-KC*NTATC*ATQRLAEFLRH
 SSNNFGPILPPTNVGSNTP-NH₂ (Acetate Salt)
 Lot. No :MTFA32213-1212
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 μ m)
 Dissolution method :100%H₂O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	35
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	35
50.00	Controller	Stop	

Chromatogram


mV

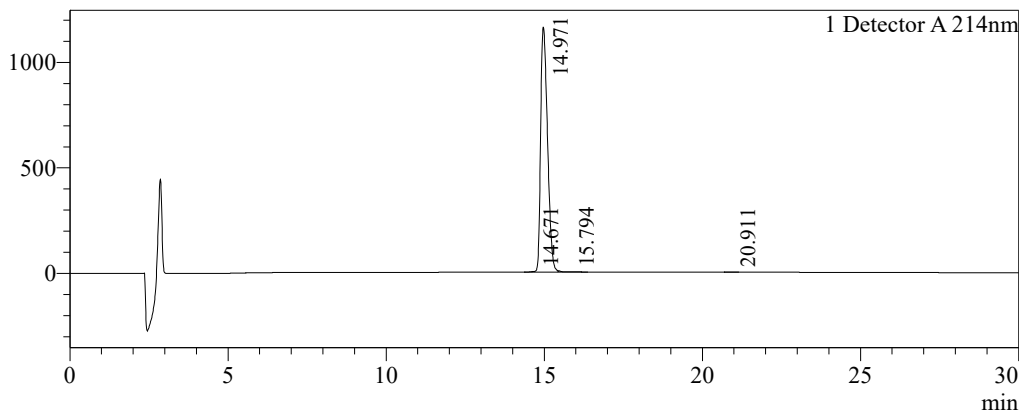

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.671	22336	2956	0.127
2	14.971	17527690	1159411	99.396
3	15.794	79733	1581	0.452
4	20.911	4509	363	0.026
Total		17634269	1164311	100.000

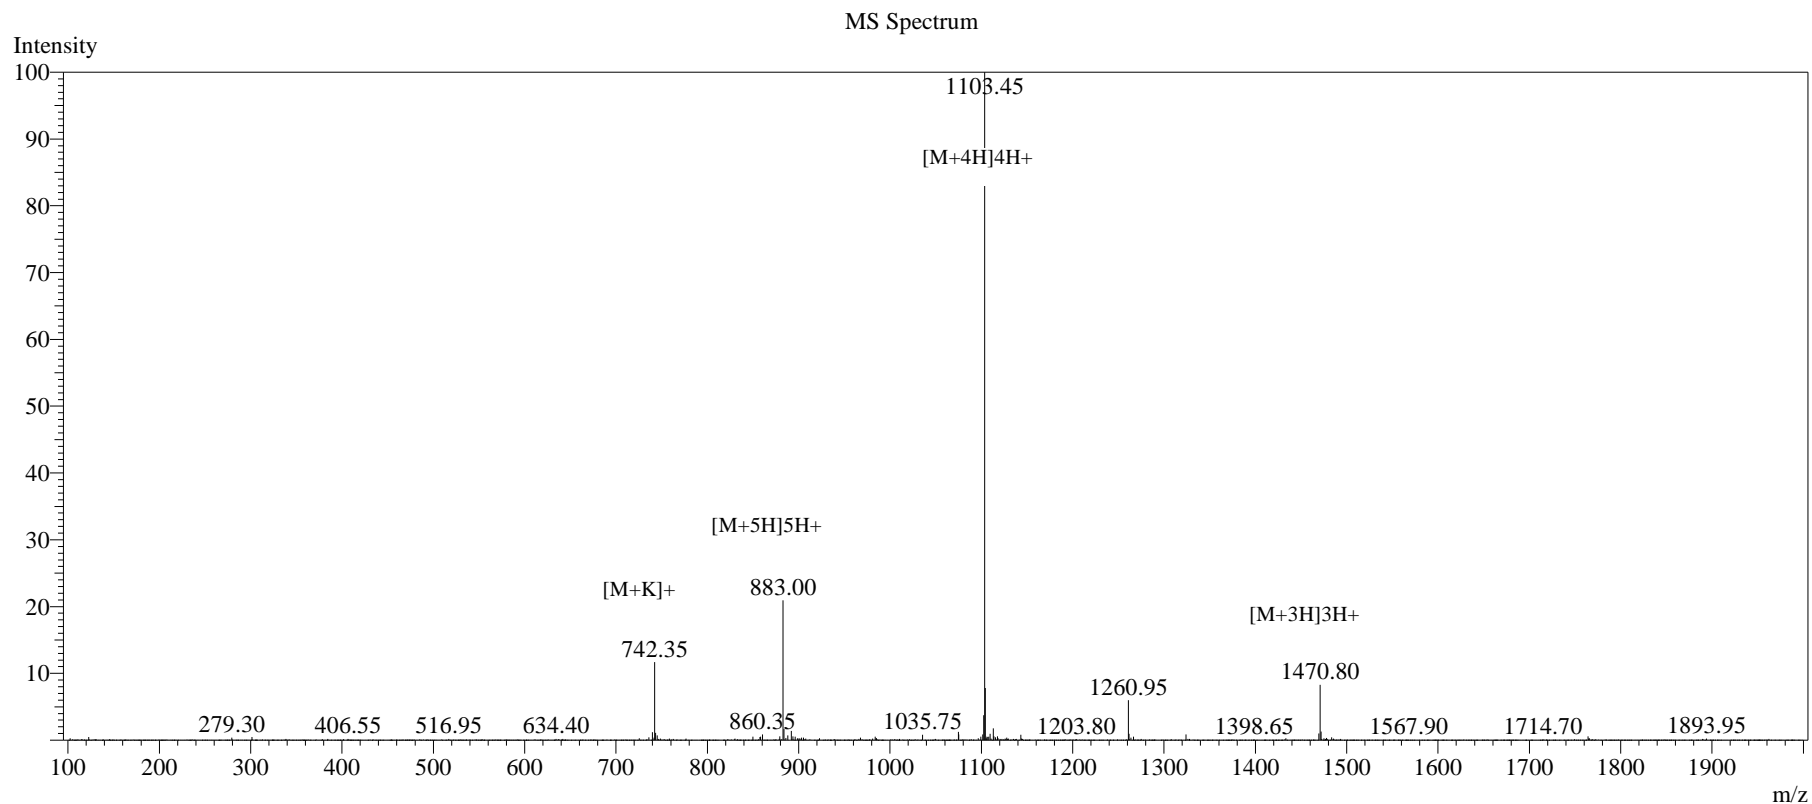

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/12/13 11:42:15	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% ME OH

Order ID	:MTFA32213
Name	:Cagrilintide
Sequence	:{Eicosanedioic acid-γ-Glu}-KC*NTATC*ATQRLAEFLRHSSNNFGPILPPTNVGSNTP-NH ₂ (Acetate Salt)
Lot.No	:MTFA32213-1212
Theoretical	:4409.01
Observed	:4409.80