


CERTIFICATE OF ANALYSIS

Product Name	Candidalysin peptide, Cat.#: 319494
Lot No.	MTFA30992-0204
Sequence	SIIGIIMGILGNIPQVIQIIMSIVKAFKGNK
Dissolution condition	100%DMSO
Length	31AA
Modification	N/A
Molecular Weight (MW)	3310.19
Storage	-20°C

Test Items	Specifications	Results
MW by MS	3310.35	Conforms
Purity by HPLC	>90%	98.285%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Apr/23/2024




Sample Information

Order ID :MTFA30992
 Name :Candidalysin peptide
 Sequence :SIIGIIMGILGNIPQVIQIIMSIVKAFKGNK
 Lot. No :MTFA30992-0204
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Phenomenex Luna® 5 µm C18(2) (4.6*250mm*5 µm)
 Dissolution method :100%DMSO
 Inj. Volume : 10ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	65
20.00	Pumps	B.Conc	85
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	65
50.00	Controller	Stop	


Chromatogram

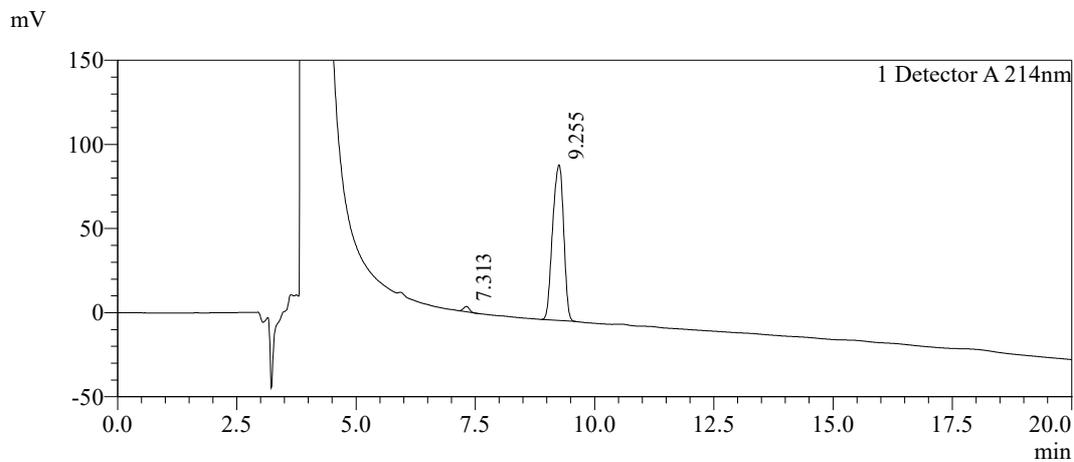

Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	7.313	25959	3121	1.715
2	9.255	1487603	92501	98.285
Total		1513561	95622	100.000

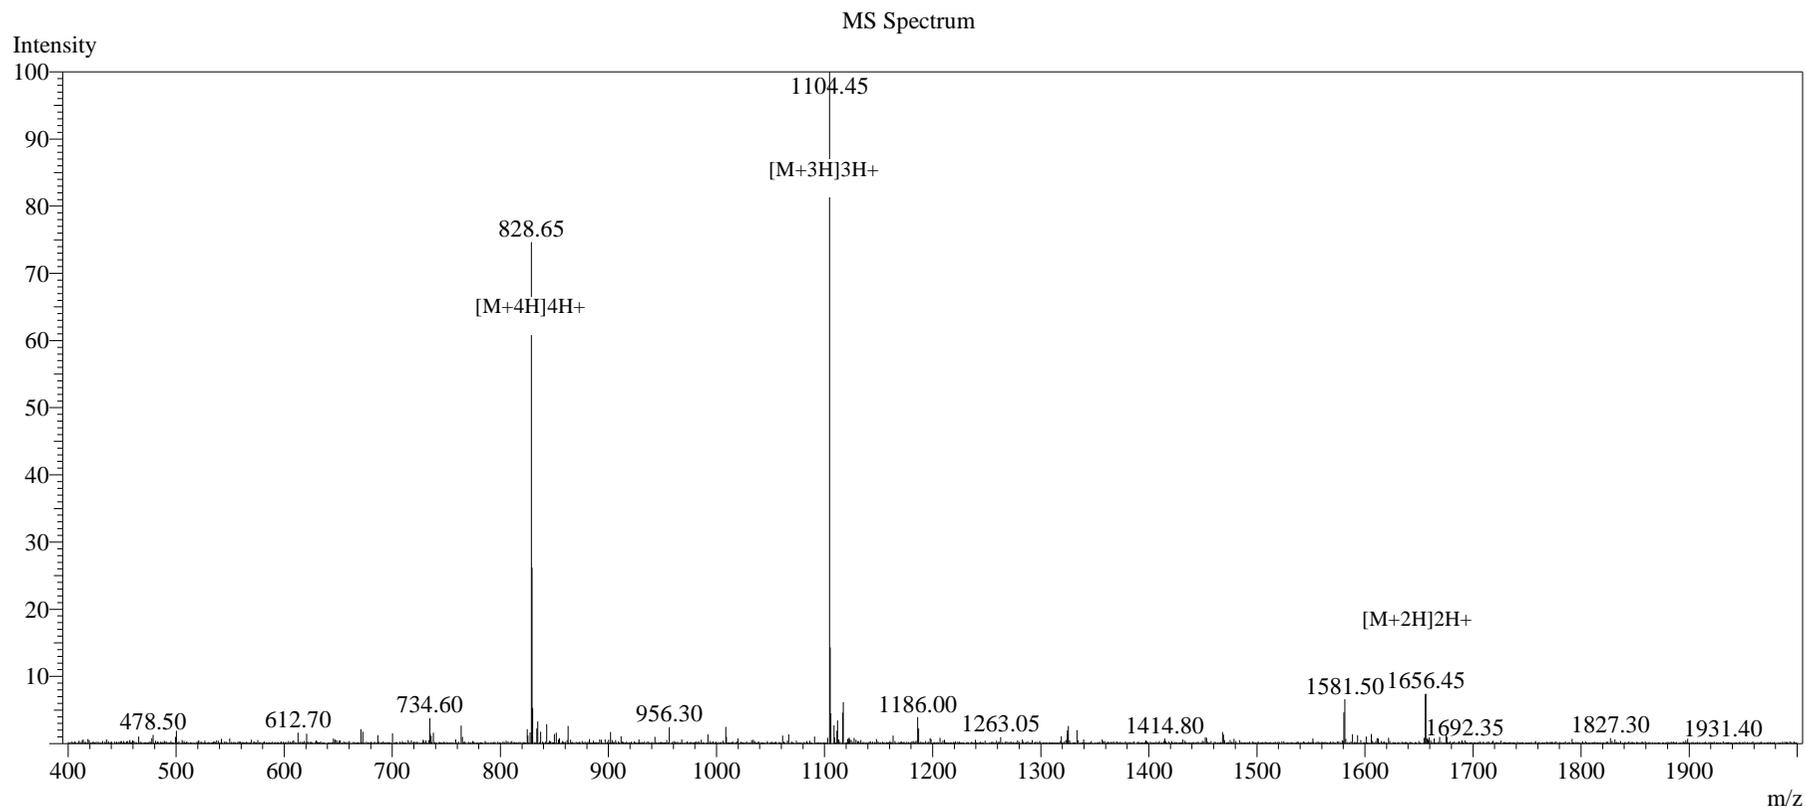

Sample Information

Dissolution method	:100%DMSO	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/04/20 11:19:51	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H2O/50% MEOH

Order ID	:MTFA30992
Name	:Candidalysin peptide
Sequence	:SIIGIIMGILGNIPQVIQIIMSIVKAFKGNK
Lot.No	:MTFA30992-0204
Theoretical	:3310.19
Observed	:3310.35