


CERTIFICATE OF ANALYSIS

Product Name	Elamipretide/SS-31, Cat.#: 318879 (TFA removed)
Lot No.	MTFA32592-0326
Sequence	D-Arg-Dmt-Lys-Phe-NH2 (Acetate Salt)
Dissolution condition	100%H2O
Length	4AA
Modification	acetate salt
Molecular Weight (MW)	639.73
Storage	-20°C

Test Items	Specifications	Results
MW by MS	639.80	Conforms
Purity by HPLC	>95%	99.320%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	1g	5.0mg*200

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department


Mar/29/2025



Sample Information

Order ID	:MTFA32592		
Name	:SS-31		
Sequence	:D-Arg-Dmt-Lys-Phe-NH2		
Lot. No	:MTFA32592-0326		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H2O		
Inj. Volume	: 10ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	15
30.00	Pumps	B.Conc	45
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	15
50.00	Controller	Stop	

Chromatogram

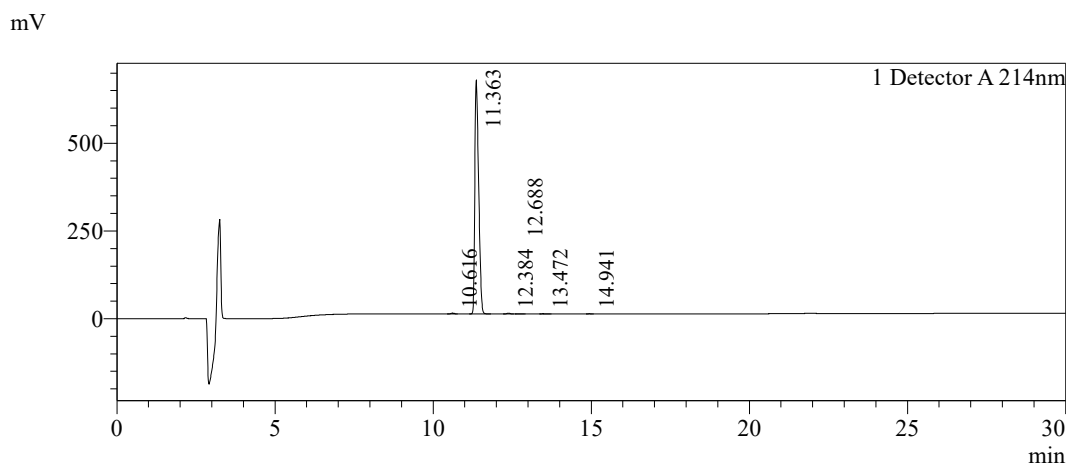


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.616	14544	2308	0.256
2	11.363	5635898	665601	99.320
3	12.384	15346	2269	0.270
4	12.688	2108	286	0.037
5	13.472	4334	570	0.076
6	14.941	2265	379	0.040
Total		5674495	671413	100.000

MS Spectrum

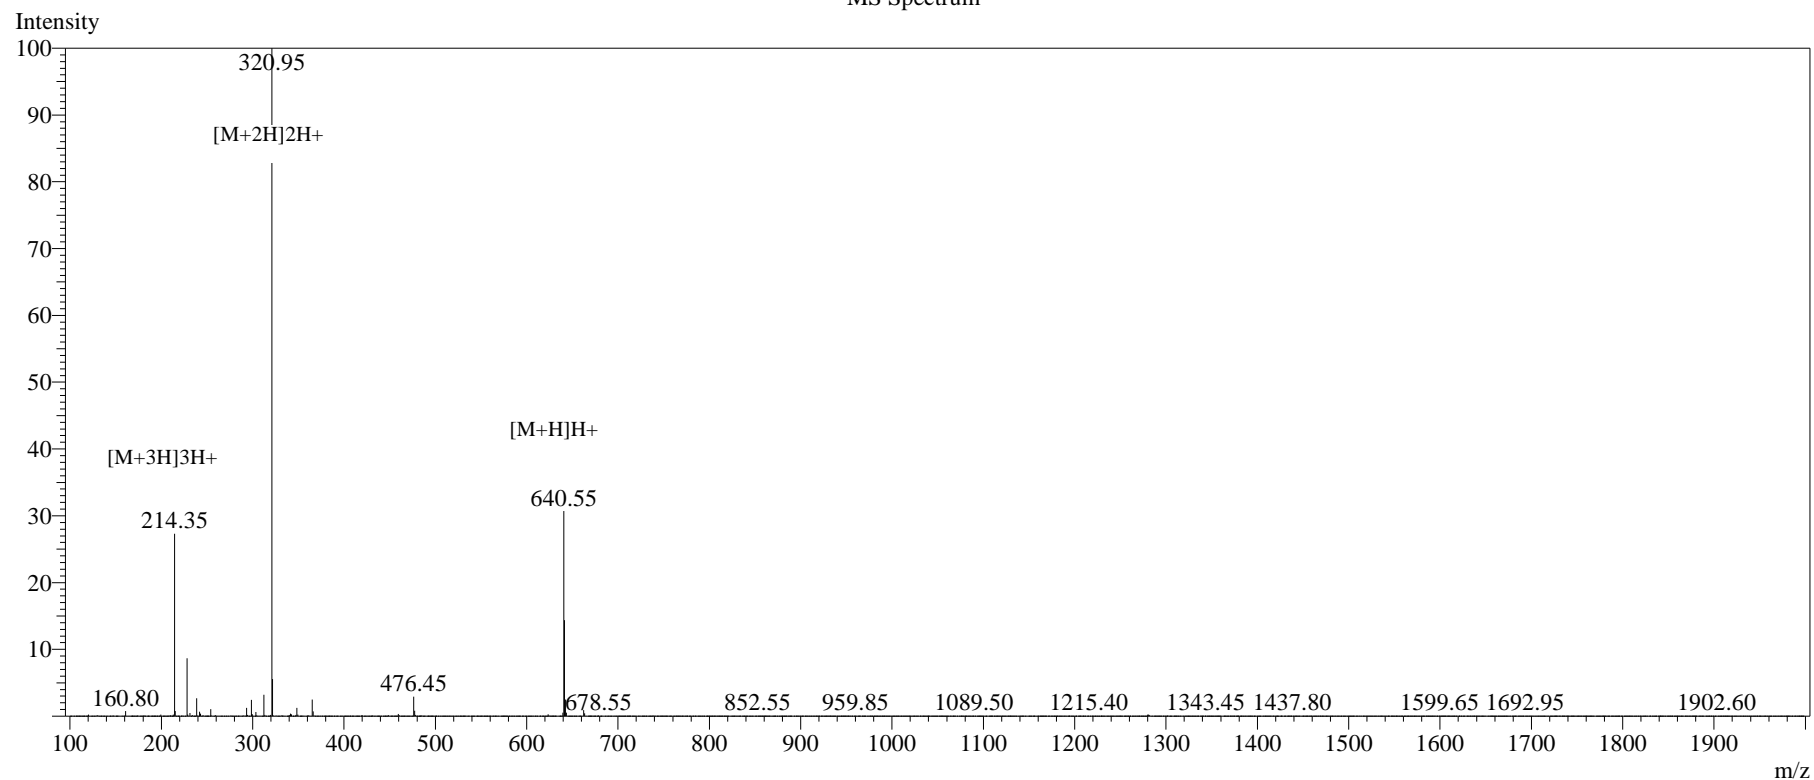

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/03/27 14:54:50	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% ME OH
Order ID	:MTFA32592				
Name	:Elamipretide/SS-31				
Sequence	:D-Arg-Dmt-Lys-Phe-NH ₂				
Lot.No	:MTFA32592-0326				
Theoretical	:639.73				
Observed	:639.90				