

## CERTIFICATE OF ANALYSIS

Product Name	H-Lys-Leu-NH <sub>2</sub> peptide, Cat.#: 300067
Lot No.	MTFA32820-250514
Sequence	KL-NH <sub>2</sub>
Dissolution condition	100%H <sub>2</sub> O
Length	AA
Modification	N/A
Molecular Weight (MW)	258.35
Storage	-20°C

Test Items	Specifications	Results
MW by MS	258.35	Conforms
Purity by HPLC	>95%	98.353%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



May/29/2025


Quality Assurance Department



### Sample Information

Order ID	:MTFA32820		
Name	:H-Lys-Leu-NH <sub>2</sub> peptide		
Sequence	:KL-NH <sub>2</sub>		
Lot. No	:MTFA32820-250514		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 µm)		
Dissolution method	:100%H <sub>2</sub> O		
Inj. Volume	: 25ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	0.1
30.00	Pumps	B.Conc	30
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	0.1
50.00	Controller	Stop	

### Chromatogram

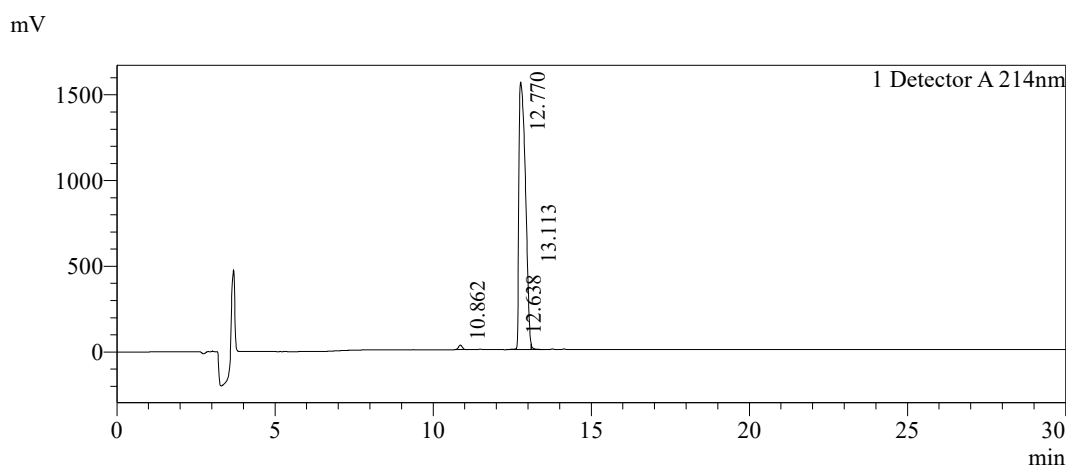


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	10.862	226203	26146	0.982
2	12.638	49300	7249	0.214
3	12.770	22649733	1559813	98.353
4	13.113	103829	27106	0.451
Total		23029066	1620314	100.000

# MS Spectrum

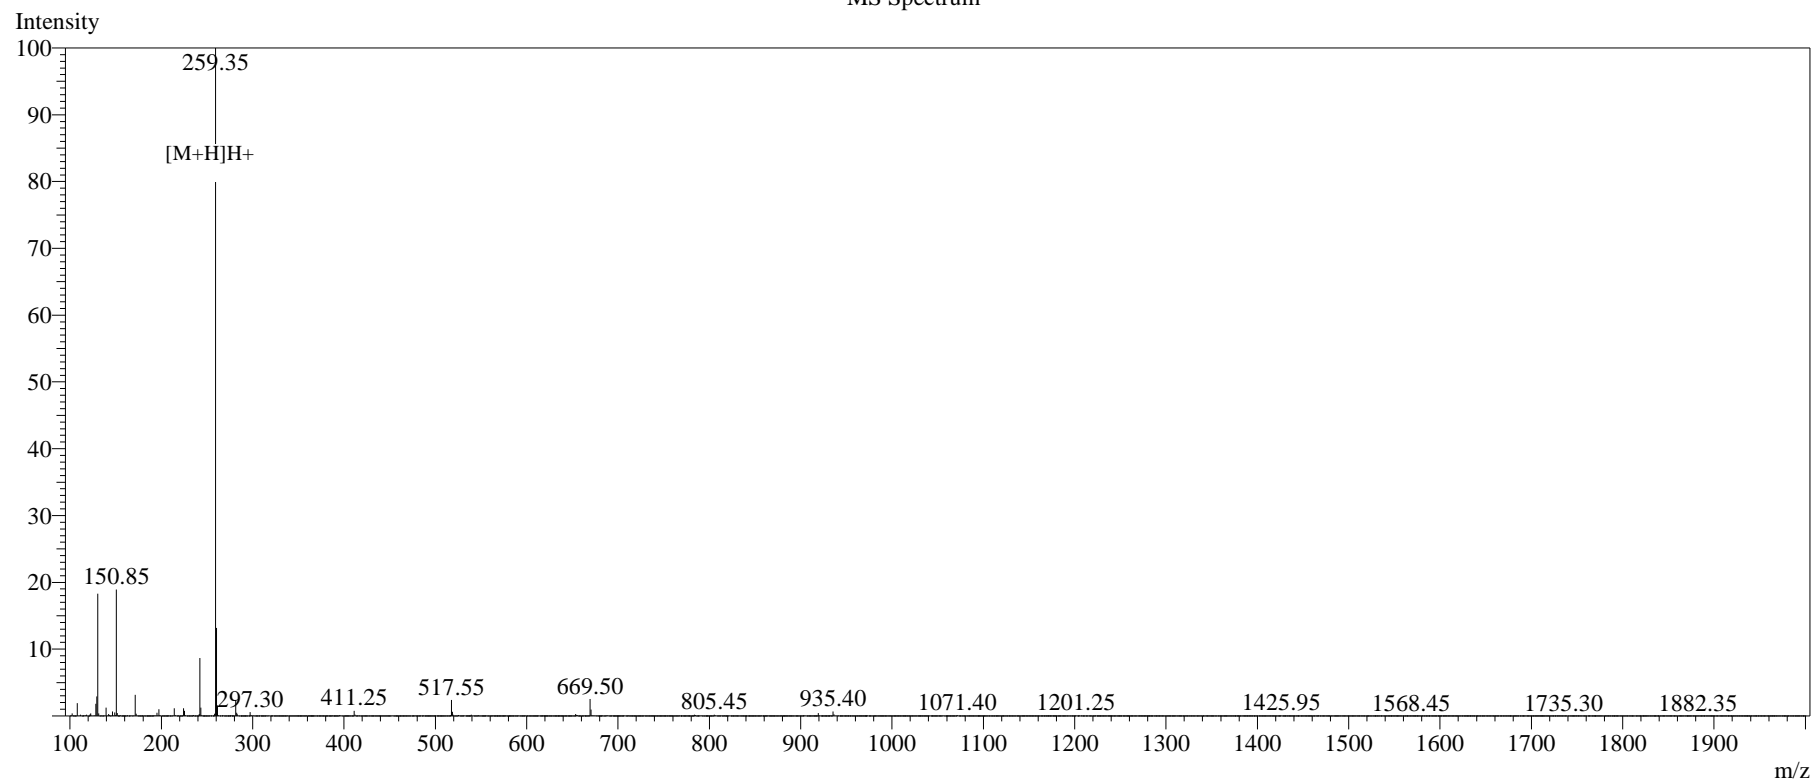

## Sample Information

Dissolution method :15%ACN+85%H<sub>2</sub>O  
 Date Acquired :2025/05/27 10:54:46  
 Injection Volume :0.2ul  
 Block Temp :200

Interface :ESI  
 Nebulizing Gas Flow :1.50L/min  
 CDL Temp :250°C  
 CDL Volt :0v

Prerod Bias :+4.5kv  
 Detector :-0.2kv  
 T.Flow :0.2ml/min  
 B.conc :50% H<sub>2</sub>O/50% MEOH

Order ID :MTFA32820  
 Name :H-Lys-Leu-NH<sub>2</sub>  
 Sequence :KL-NH<sub>2</sub>  
 Lot.No :MTFA32820-250514  
 Theoretical :258.35  
 Observed :258.35