

---

**CERTIFICATE OF ANALYSIS**

<b>Product Name</b>	Peptide T7 with N-Cys, Cat.#: 318911
<b>Lot No.</b>	MTFA32318-0109
<b>Sequence</b>	CHAIYPRH
<b>Dissolution condition</b>	100%H <sub>2</sub> O
<b>Length</b>	8AA
<b>Modification</b>	N/A
<b>Molecular Weight (MW)</b>	996.15
<b>Storage</b>	-20°C


---

<b>Test Items</b>	<b>Specifications</b>	<b>Results</b>
<b>MW by MS</b>	996.45	Conforms
<b>Purity by HPLC</b>	>95%	98.667%
<b>Peptide content</b>	N/A	N/A
<b>Moisture content</b>	N/A	N/A
<b>Acetic acid content</b>	N/A	N/A
<b>Appearance</b>	White to off-white lyophilized powder	Conforms
<b>Quantity</b>	100mg	5.0mg*20

---

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Jan/13/2025




### Sample Information

Order ID :MTFA32318  
 Name :Peptide T7 with N-Cys  
 Sequence :CHAIYPRH  
 Lot. No :MTFA32318-0109  
 Pump A :0.1%Trifluoroacetic in 100% water  
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile  
 Total Flow :1ml/min  
 Wavelength :214nm  
 Analytical column type :Kromasil 100-5-C18 (4.6\*250mm\*5 µm)  
 Dissolution method :100%H2O  
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	5
30.00	Pumps	B.Conc	35
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	5
50.00	Controller	Stop	

### Chromatogram

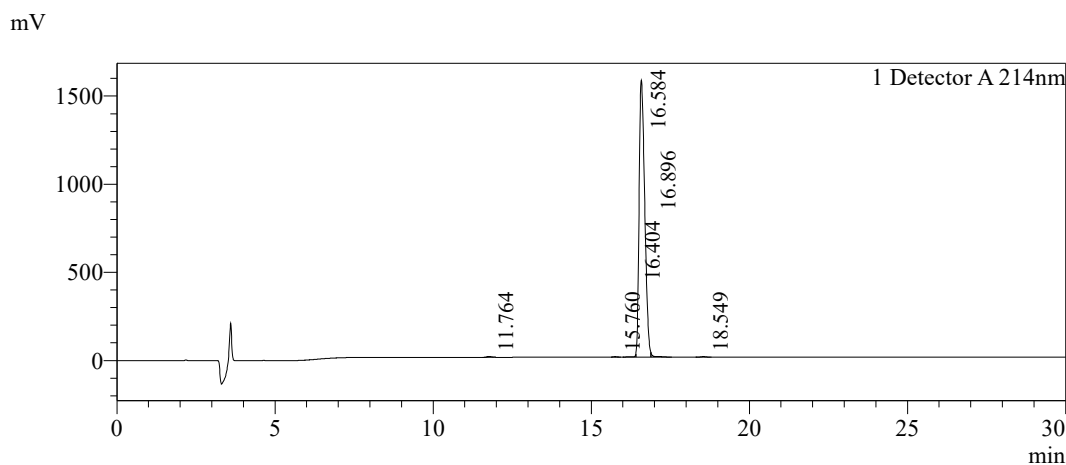


### Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	11.764	52017	4993	0.264
2	15.760	18639	2422	0.095
3	16.404	45153	11215	0.229
4	16.584	19427783	1569949	98.667
5	16.896	113116	21410	0.574
6	18.549	33635	3048	0.171
Total		19690343	1613038	100.000

## MS Spectrum

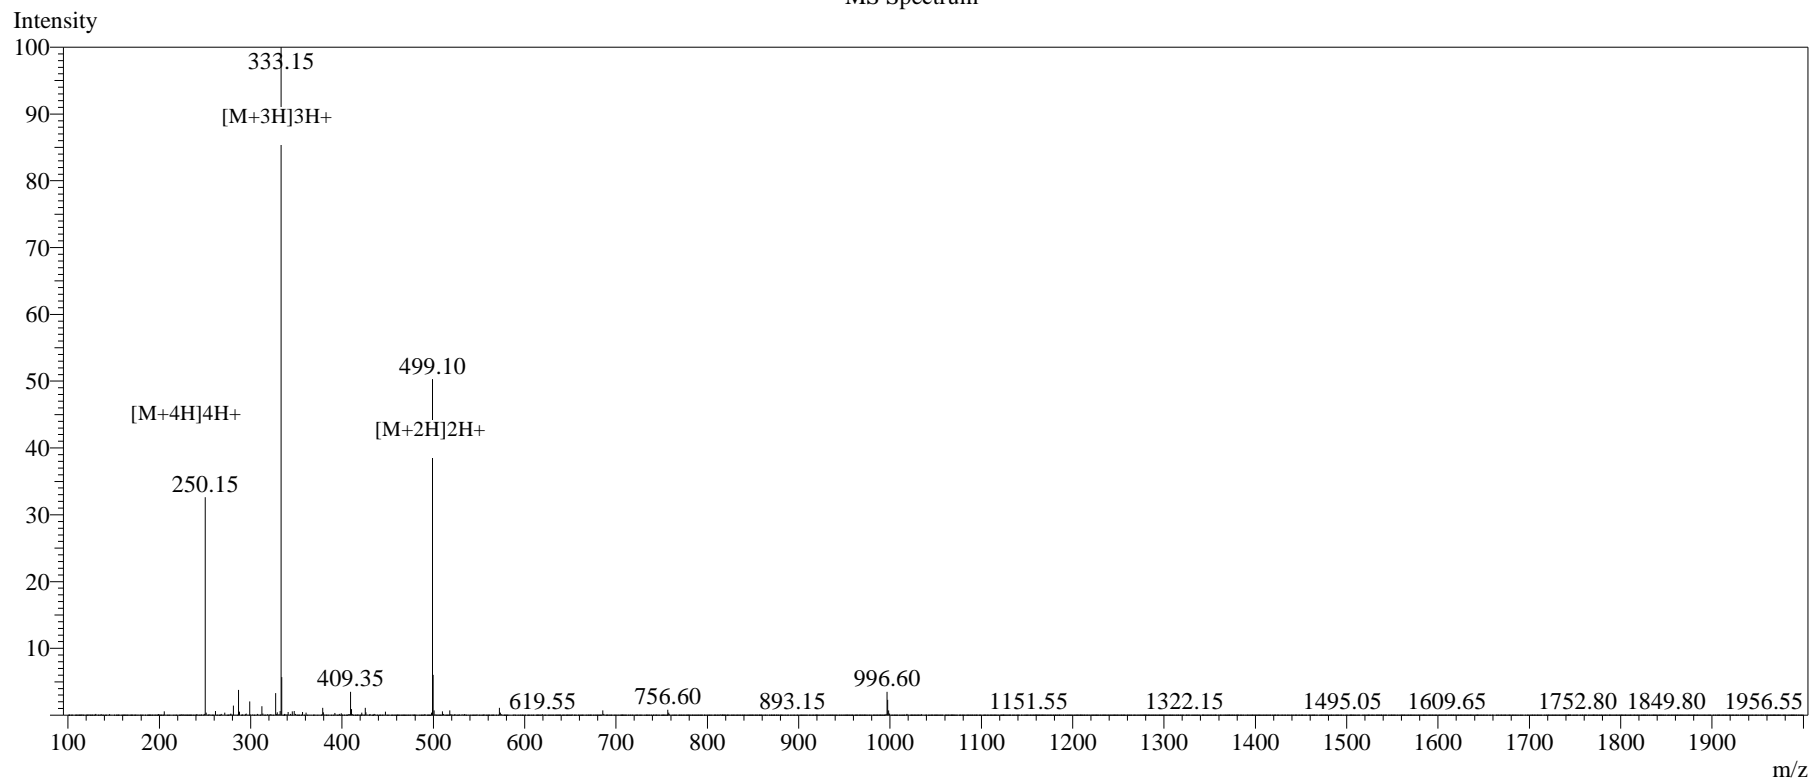

## Sample Information

Dissolution method	:15% ACN+85% H <sub>2</sub> O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2025/01/10 16:10:06	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H <sub>2</sub> O/50% MEOH

Order ID	:MTFA32318
Name	:Peptide T7 with N-Cys
Sequence	:CHAIYPRH
Lot.No	:MTFA32318-0109
Theoretical	:996.15
Observed	:996.45