

CERTIFICATE OF ANALYSIS

Product Name	R-E-D-V peptide, Cat.#: 302082 (TFA removed)
Lot No.	MTFA31196-0401
Sequence	REDV (Acetate Salt)
Dissolution condition	100%H ₂ O
Length	4AA
Modification	Acetate salts
Molecular Weight (MW)	517.53
Storage	-20°C

Test Items	Specifications	Results
MW by MS	517.45	Conforms
Purity by HPLC	>95%	96.902%
Peptide content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	25mg	5.0mg*5

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Quality Assurance Department

Apr/10/2024




Sample Information

Order ID :MTFA31196
 Name :REDV
 Sequence :REDV (Acetate Salt)
 Lot. No :MTFA31196-0401
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Phenomenex Luna® 5 µm C18 (2) (4.6*250mm*5 µm)
 Dissolution method :100%H2O
 Inj. Volume : 4ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	0.1
20.00	Pumps	B.Conc	20
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	0.1
50.00	Controller	Stop	

Chromatogram

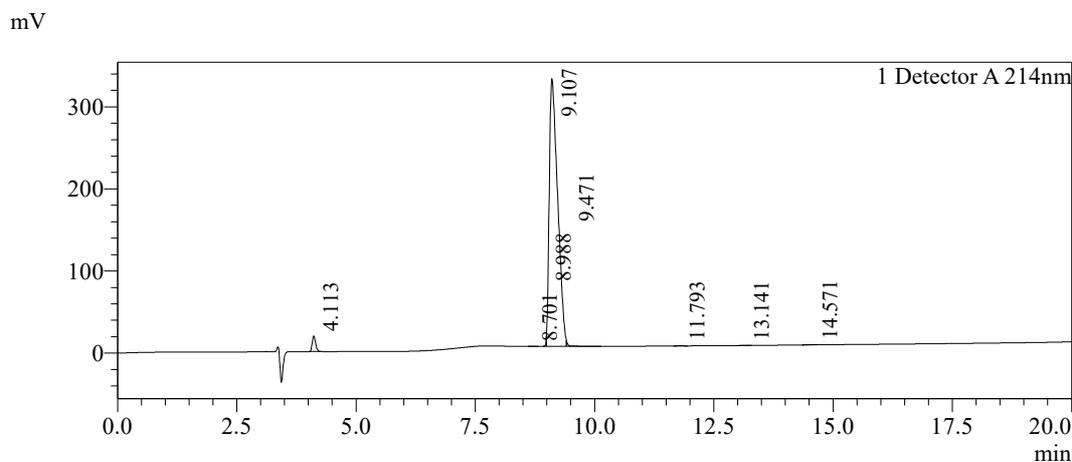


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	4.113	92081	18718	2.248
2	8.701	663	120	0.016
3	8.988	12333	6457	0.301
4	9.107	3969148	325428	96.902
5	9.471	17387	993	0.424
6	11.793	2181	282	0.053
7	13.141	1288	170	0.031
8	14.571	950	96	0.023
Total		4096031	352263	100.000

MS Spectrum

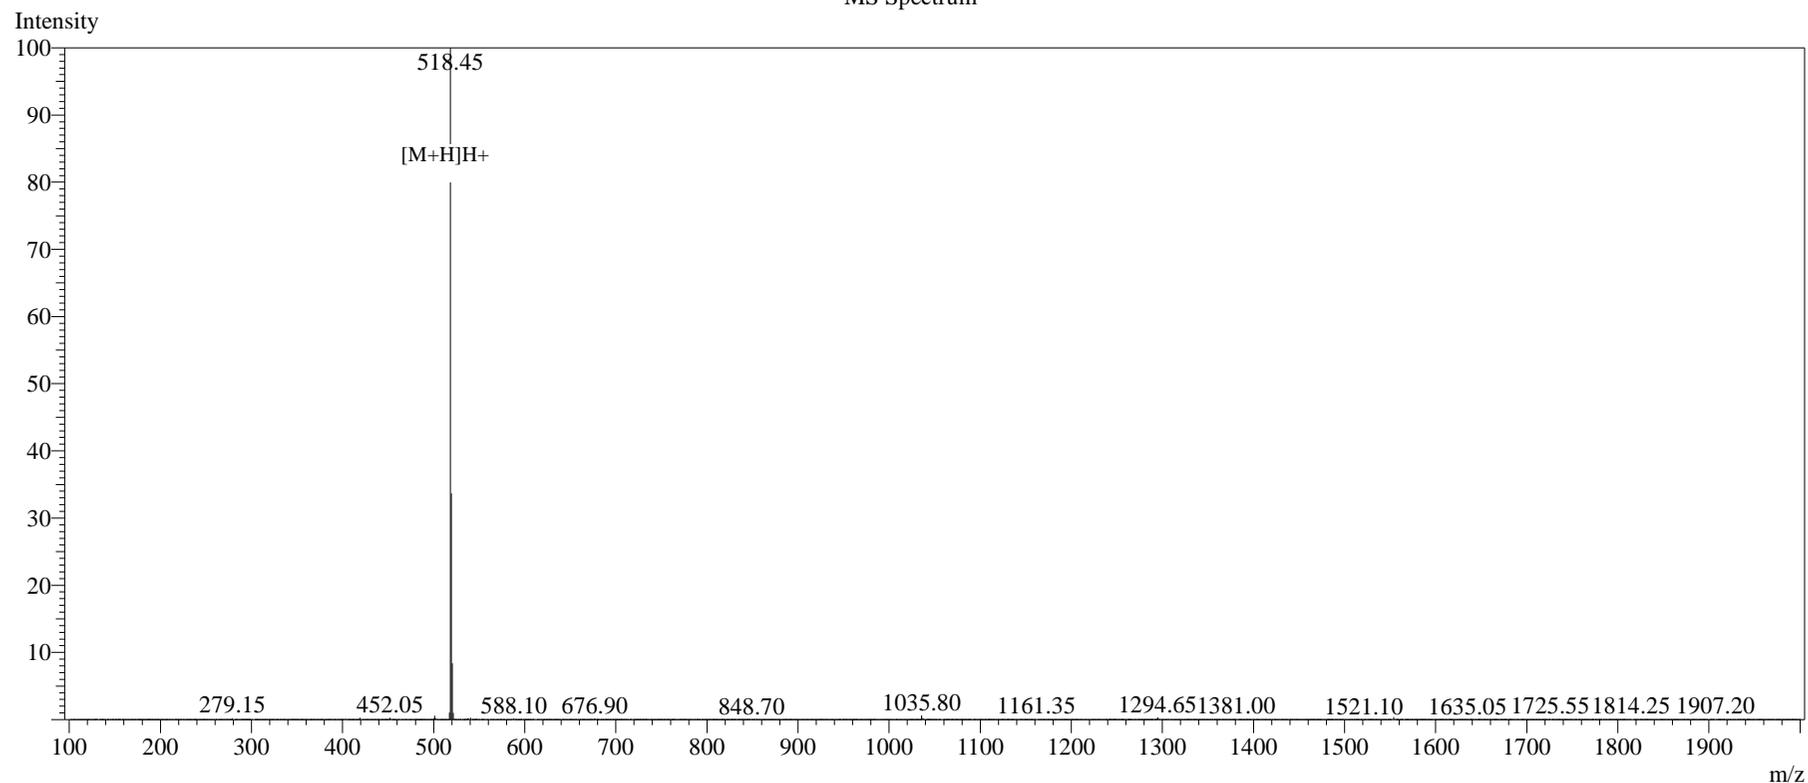

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2024/04/07 13:52:06	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFA31196
Name	:REDV
Sequence	:REDV (Acetate Salt)
Lot.No	:MTFA31196-0401
Theoretical	:517.53
Observed	:517.45