

CERTIFICATE OF ANALYSIS

Product Name VCT-VT2 (Cat.#: 309549)

Lot No. MTFA30608-3-1019

Sequence FLPIIGKLLSG

Dissolution condition 100%H2O

Length 11AA

Modification N/A

Molecular Weight (MW) 1157.45

Storage -20°C

Test Items	Specifications	Results
MW by MS	1157.50	Conforms
Purity by HPLC	>95%	99.569%
Peptide Content	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	20mg	5.0mg*4

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:

Nov/09/2023



Sample Information

Order ID :MTFA30608-3
Name :VCT-VT2
Sequence :FLPIIGKLLSG
Lot. No :MTFA30608-3-1019

Pump A :0.1%Trifluoroacetic in 100% water Pump B :0.1%Trifluoroacetic in 100% acetonitrile

Total Flow :1ml/min Wavelength :214nm

Analytial column type :Phenomenex Luna® 5 μm C18(2) (4.6*250mm*5 μm)

Dissolution method :100%H2O


Inj. Volume : 20ul
Time Module

Time	Module	Action	Value
0.01	Pumps	B.Conc	30
30.00	Pumps	B.Conc	60
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	30
50.00	Controller	Ston	

50.00 Controller Stop

Chromatogram



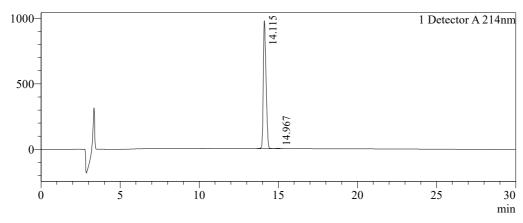


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	14.115	11828230	972788	99.569
2	14.967	51169	3135	0.431
Total		11879399	975922	100.000



MS Spectrum

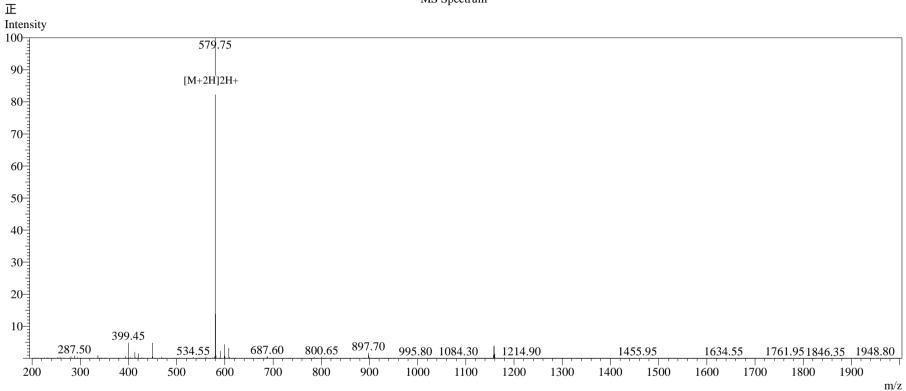

Sample Information

Dissolution method	:15% ACN+85% H2O	Interface	:ESI	Prerod Bias	:+4.5kv :-0.2kv
Date Acquired	:2023/11/02 13:32:20	Nebulizing Gas Flow	:1.50L/min	Detector	
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID :MTFA30608-3
Name :VCT-VT2
Sequence :FLPIIGKLLSG
Lot.No :MTFA30608-3-1019
Theoretical :1157.45

Theoretical :1157.45 Observed :1157.50