
CERTIFICATE OF ANALYSIS

Product Name	Vasodilator peptide 1095.6 Da, Cat.#: 305478
Lot No.	MTFB20358-251209
Sequence	{Pyr}-GRPPGPPIPP
Dissolution condition	100%H2O
Modification	N/A
Molecular Weight (MW)	1095.27
Storage	-20°C

Test Items	Specifications	Results
MW by MS	1095.50	Conforms
Purity by HPLC	>95%	95.651%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10 mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by: 
Quality Assurance Department

Jan/13/2026




Sample Information


Order ID	:MTFB20358		
Name	:Vasodilator peptide 1095.6 Da		
Sequence	:{Pyr}-GRPPGPIPP		
Lot. No	:MTFB20358-251209		
Pump A	:0.1%Trifluoroacetic in 100% water		
Pump B	:0.1%Trifluoroacetic in 100% acetonitrile		
Total Flow	:1ml/min		
Wavelength	:214nm		
Analytical column type	:Kromasil 100-5-C18 (4.6*250mm*5 μm)		
Dissolution method	:100%H2O		
Inj. Volume	: 30ul		
Time	Module	Action	Value
0.01	Pumps	B.Conc	10
30.00	Pumps	B.Conc	40
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	10
50.00	Controller	Stop	

Chromatogram

mV

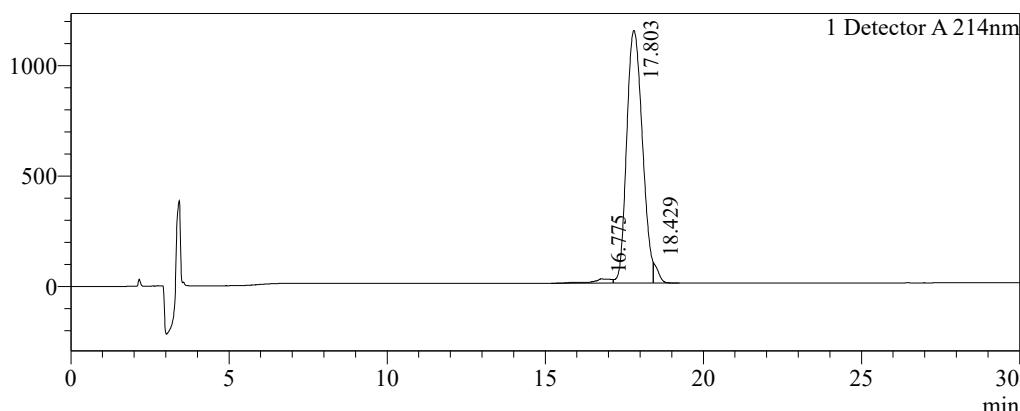
Peak Table
Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	16.775	818271	19685	1.981
2	17.803	39514737	1143776	95.651
3	18.429	978444	91916	2.368
Total		41311452	1255376	100.000

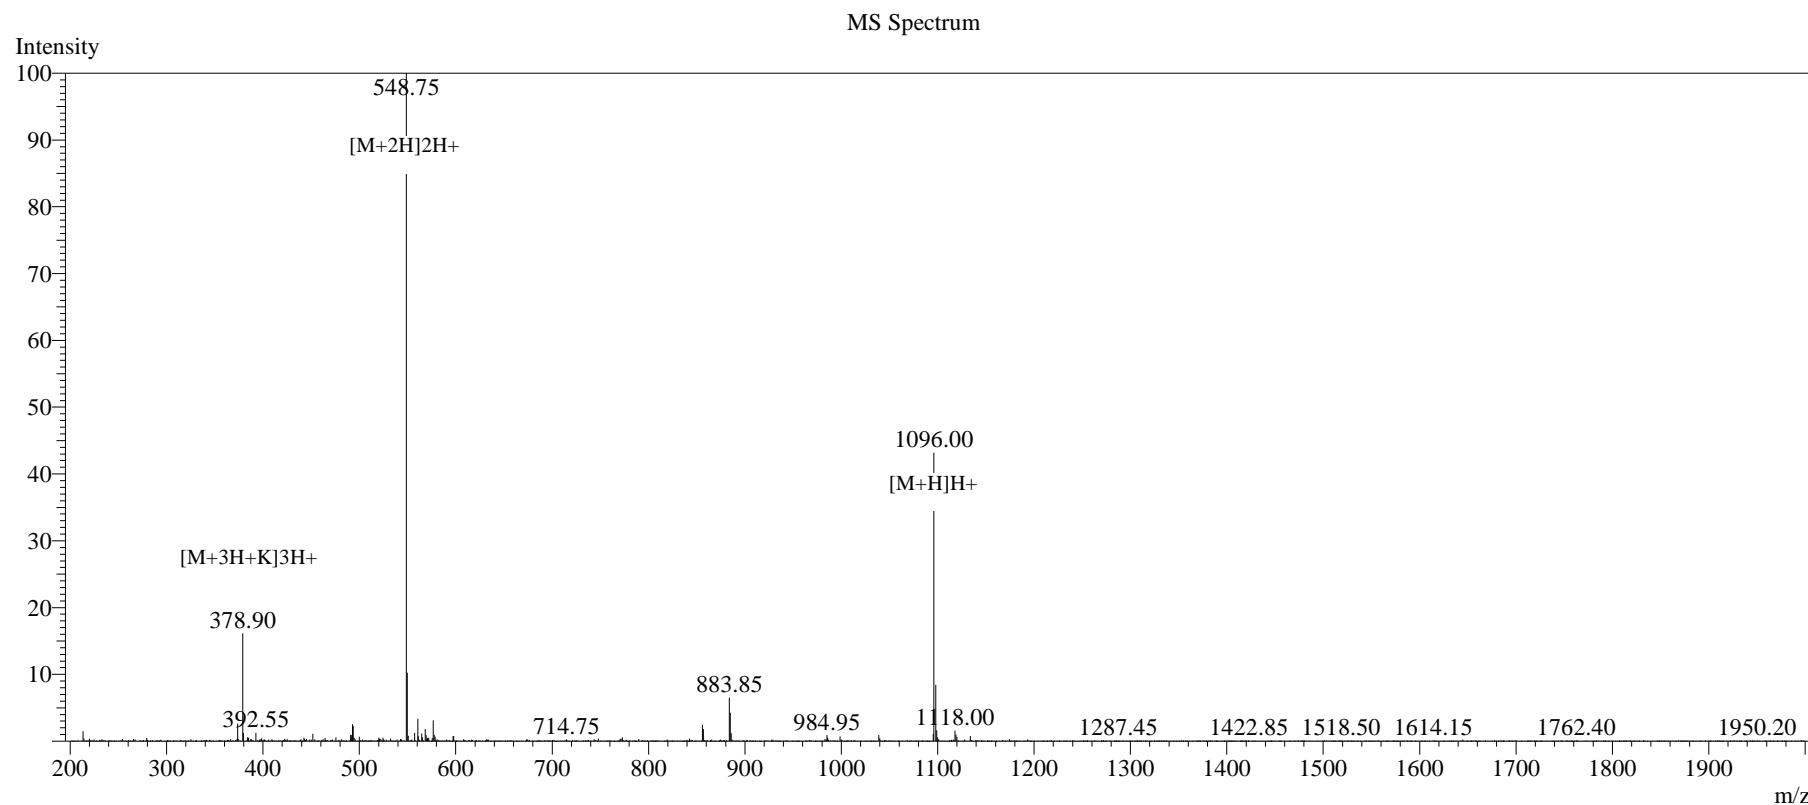

Sample Information

Dissolution method	:15%ACN+85%H2O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/01/08 10:46:18	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50%H2O/50%MEOH

Order ID	:MTFB20358
Name	:Vasodilator peptide 1095.6 Da
Sequence	:{Pyr}-GRPPGPPIPP
Lot.No	:MTFB20358-251209
Theoretical	:1095.27
Observed	:1095.50