
CERTIFICATE OF ANALYSIS

Product Name	human Histatin 5 peptide, Cat.#: 313959 (TFA Removed)
Lot No.	MTFB20540-260205
Sequence	DSHAKRHHGYKRKFHEKHHSRGGY (Acetate Salt)
Dissolution condition	100%H ₂ O
Modification	Acetate Salt
Molecular Weight (MW)	3036.32
Storage	-20°C

Test Items	Specifications	Results
MW by MS	3036.90	Conforms
Purity by HPLC	>95%	95.298%
Endotoxin Content	N/A	N/A
TFA solubility	N/A	N/A
Moisture content	N/A	N/A
Acetic acid content	N/A	N/A
Appearance	White to off-white lyophilized powder	Conforms
Quantity	10 mg	5.0mg*2

NovoPro Bioscience Inc. (hereafter NovoPro) warrants material of said quality at the time of sale. It is the sole responsibility of the customers to determine the adequacy of all materials for any intended or specific purpose or use. NovoPro's sole obligation is to replace the material up to the extent of the purchase price. This warranty applies only to products in original packaging and does not apply to a product which has been tampered with or altered in any way in or which has been misused or damaged by accident or negligence. All claims must be received writing (by fax or email) within 30 days from date when product arrive at the destination city and failure to do so shall constitute a waiver by customers for any and all such claims.

Certified by:



Feb/12/2026

Quality Assurance Department




Sample Information

Order ID :MTFB20540
 Name :human Histatin 5 peptide
 Sequence :DSHAKRHHGGYKRFHEKHHSHRGY (Acetate Salt)
 Lot. No :MTFB20540-260205
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetonitrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type :Kromasil 100-5-C18 (4.6*250mm*5 µm)
 Dissolution method :100%H₂O
 Inj. Volume : 25ul

Time	Module	Action	Value
0.01	Pumps	B.Conc	10
30.00	Pumps	B.Conc	40
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	10
50.00	Controller	Stop	

Chromatogram

mV

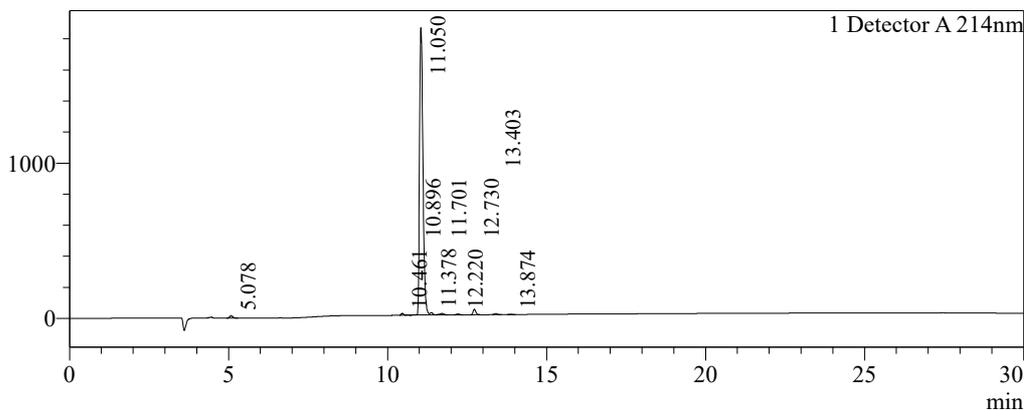


Peak Table

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	5.078	106885	15033	0.741
2	10.461	69815	11510	0.484
3	10.896	9742	1364	0.068
4	11.050	13745733	1850149	95.298
5	11.378	88464	14585	0.613
6	11.701	82708	9357	0.573
7	12.220	43097	5504	0.299
8	12.730	217856	35585	1.510
9	13.403	47250	7758	0.328
10	13.874	12438	2006	0.086
Total		14423986	1952851	100.000

MS Spectrum

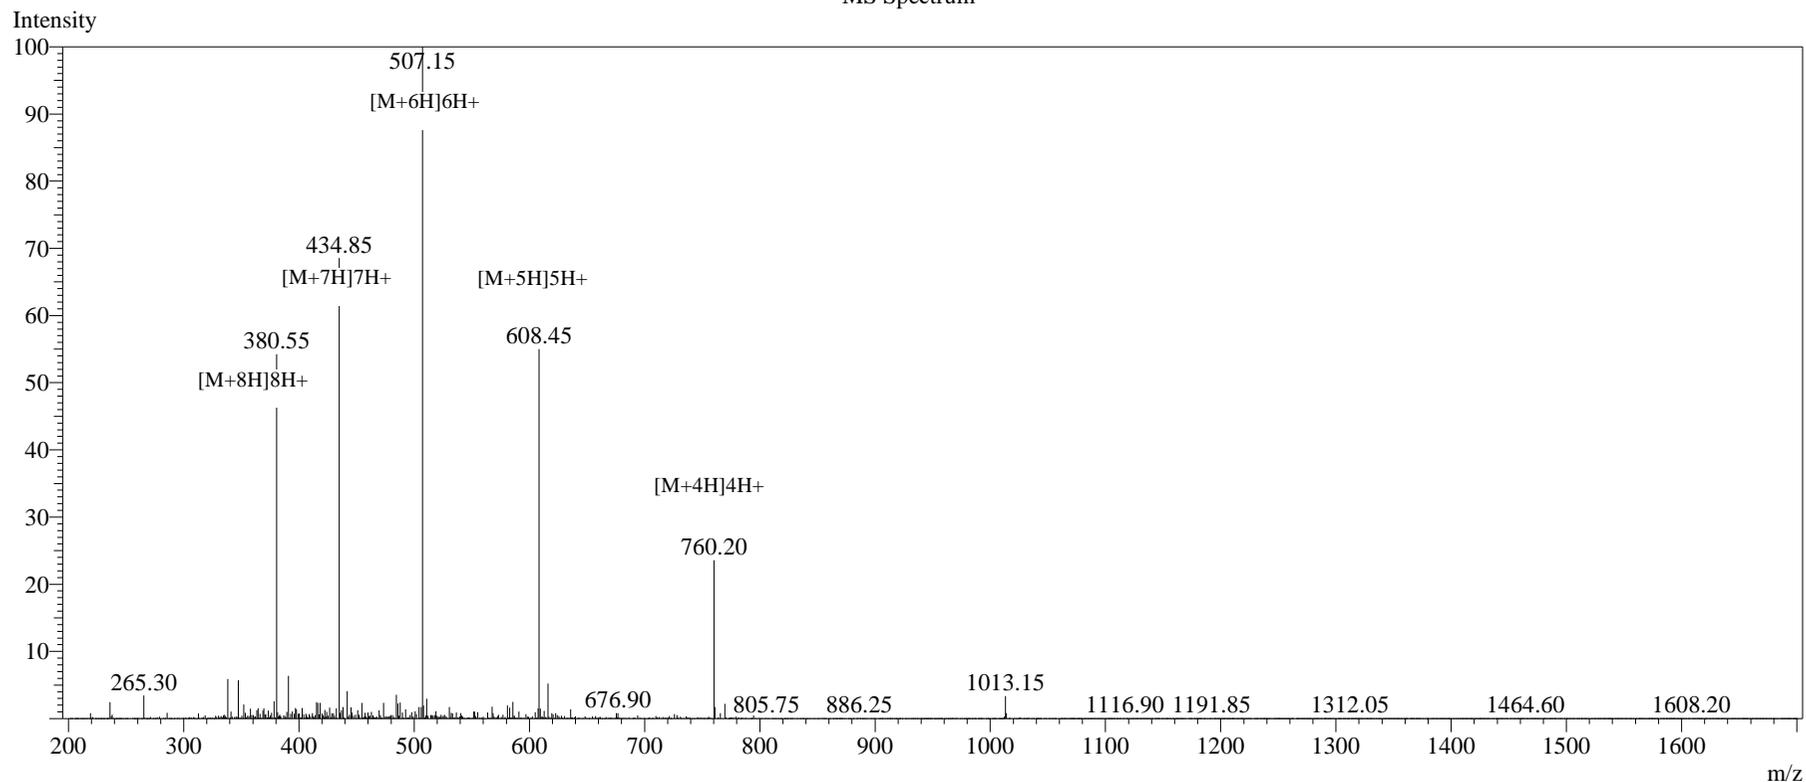

Sample Information

Dissolution method	:15% ACN+85% H ₂ O	Interface	:ESI	Prerod Bias	:+4.5kv
Date Acquired	:2026/02/10 15:39:37	Nebulizing Gas Flow	:1.50L/min	Detector	:-0.2kv
Injection Volume	:0.2ul	CDL Temp	:250°C	T.Flow	:0.2ml/min
Block Temp	:200	CDL Volt	:0v	B.conc	:50% H ₂ O/50% MEOH

Order ID	:MTFB20540
Name	:human Histatin 5 peptide
Sequence	:DSHAKRHHGYKRFHEKHHSHRGY (Acetate Salt)
Lot.No	:MTFB20540-260205
Theoretical	:3036.32
Observed	:3036.90